




GENERAL INFORMATION


Medical Equipment Washing & Decontamination Systems



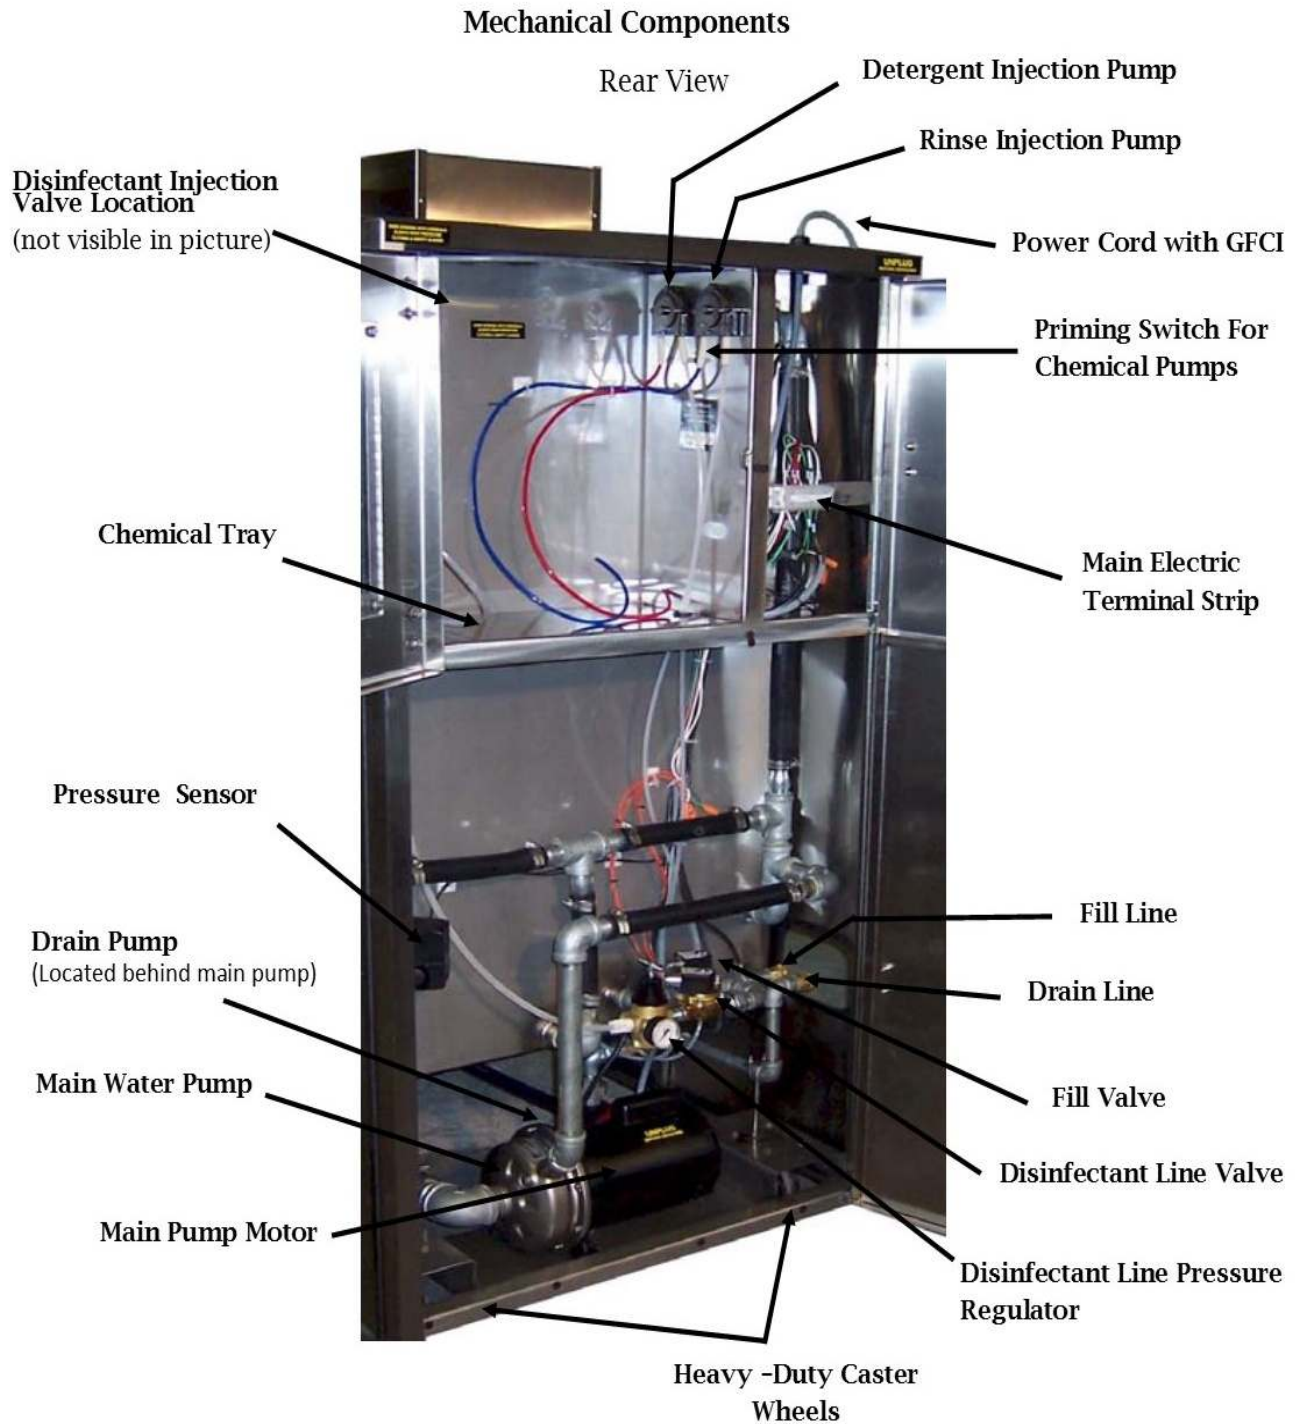


GENERAL INFORMATION FILTERS & SCREENS

IT IS RECOMMENDED THAT YOU CHECK THE FILTERS DAILY FOR DEBRIS
AND CLEAN THEM OFTEN.

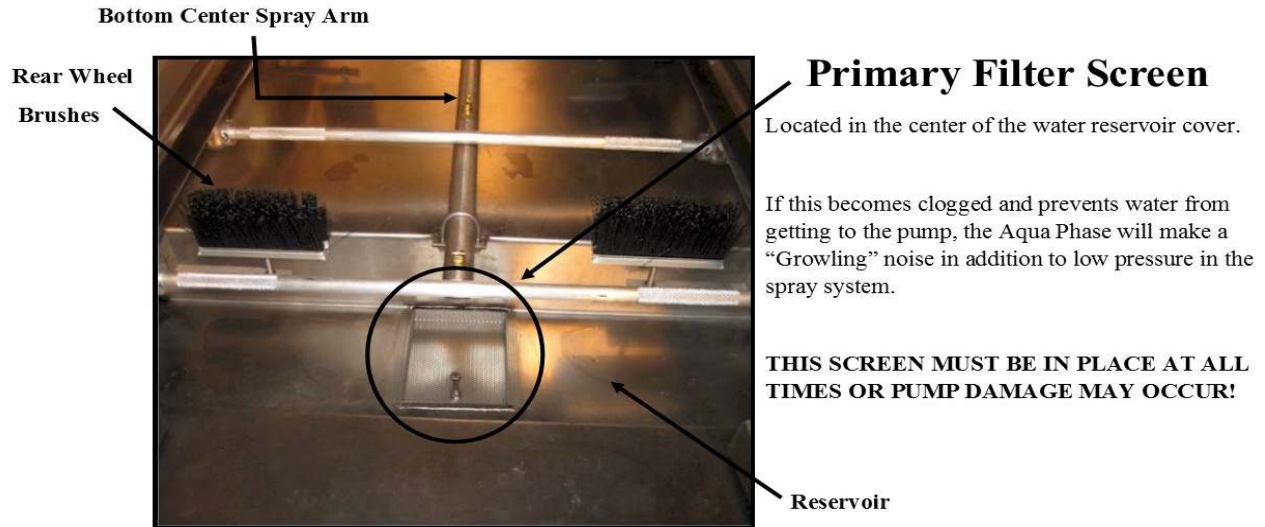

Primary Filter Screen (Removed)

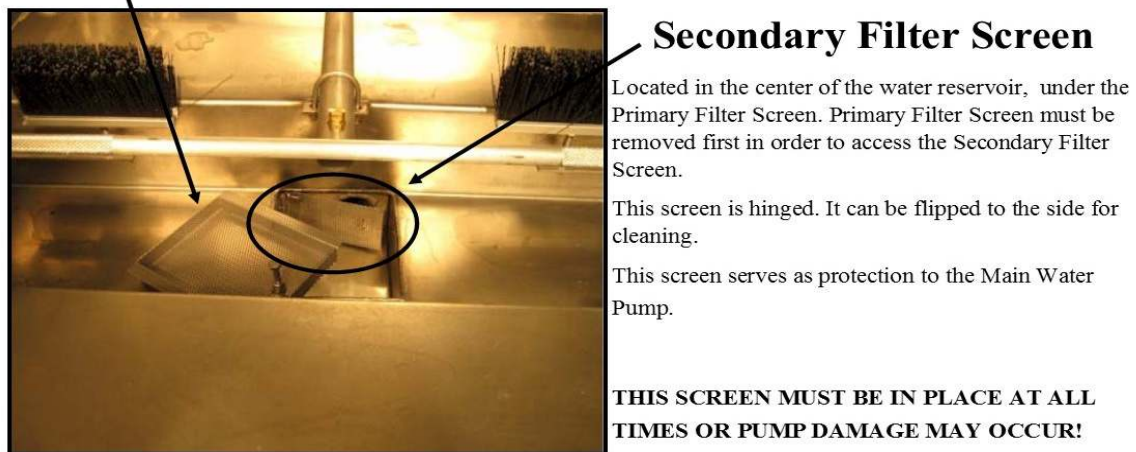

IF YOUR UNIT DOES NOT HAVE THE FILTER SCREENS SEATED PROPERLY, IN THEIR PLACE AT ALL TIMES, YOU CAN EXPECT THE SPRAY NOZZLES TO BECOME CLOGGED.